


Certificate

TaiDoc Technology Corp.

using

Immunoassay on TD-4611

participated in the IFCC HbA1c Certification Programme to demonstrate
 traceability to the IFCC Reference Measurement Procedure and
 performed as shown below.

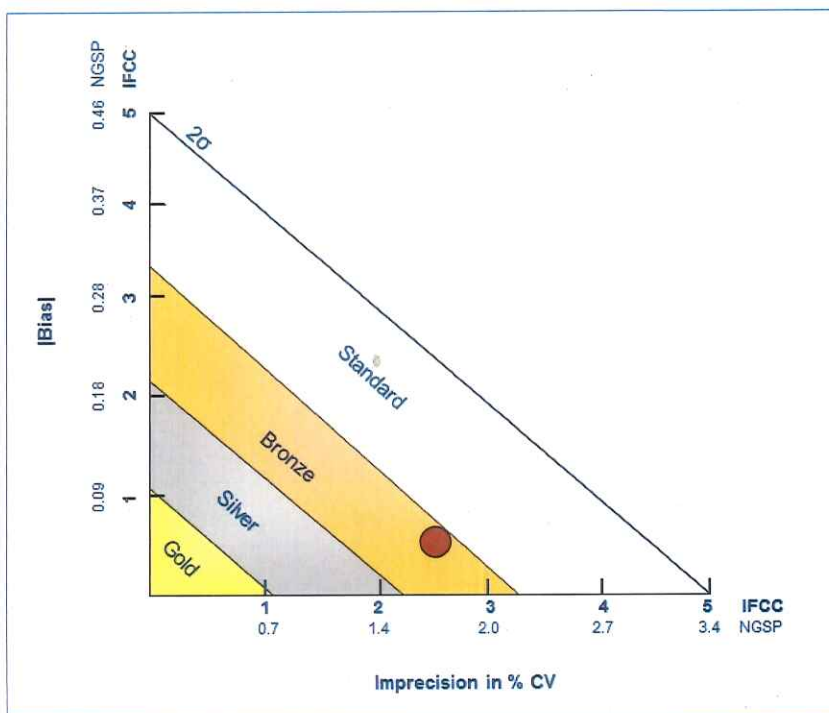

Total Error =	3.1 mmol/mol
Bias =	0.6 mmol/mol
Imprecision =	2.5 %
Grade =	Bronze

Criteria derived from the IFCC model for Quality Targets HbA1c (Clin Chem 2015;61:752-59)

Date of Certification: 01 January 2018

Date of Expiry: 01 January 2019



IFCC Network Coordinator
 Dr. C.W. Weykamp